


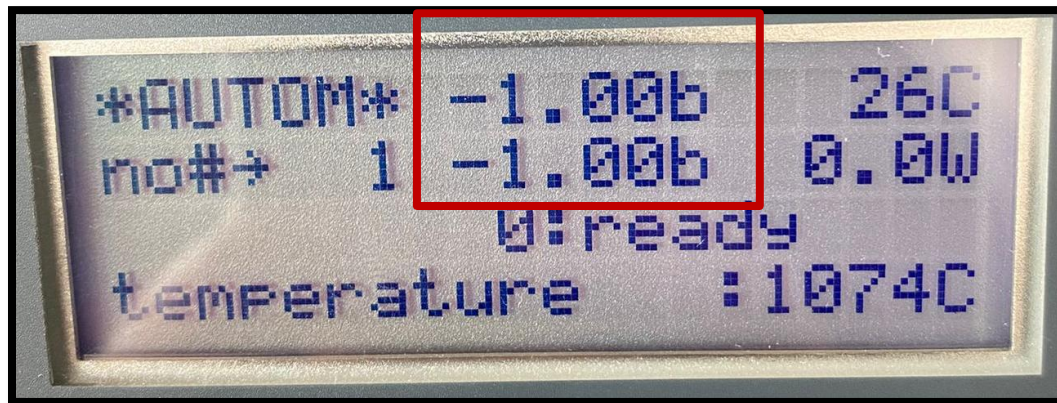
Identifier	<h1>Service Document</h1>	
Service SH		
<h2>T-H-40-01 How to Reset the Pressure Sensors VPC 40</h2>		Römerstr. 21 D – 71296 Heimsheim Tel.: + 49(0)7033-309878-41 service@schultheiss-gmbh.de http://www.schultheiss-gmbh.de

Apply for:

Machine Type	Version	Year
VPC 40	All	Since Release

Problem



How to Reset the Pressure Sensors VPC 40





Prerequisites


- Connect Pressure Gas
- Opened the valve so the gas can flow

Procedure

- Switch ON the machine
- Wait until the Self-test is completed
- Press  'M' to enter the Automatic Mode
- Press and Hold  'Down' until you reach the 'Sensor' menu

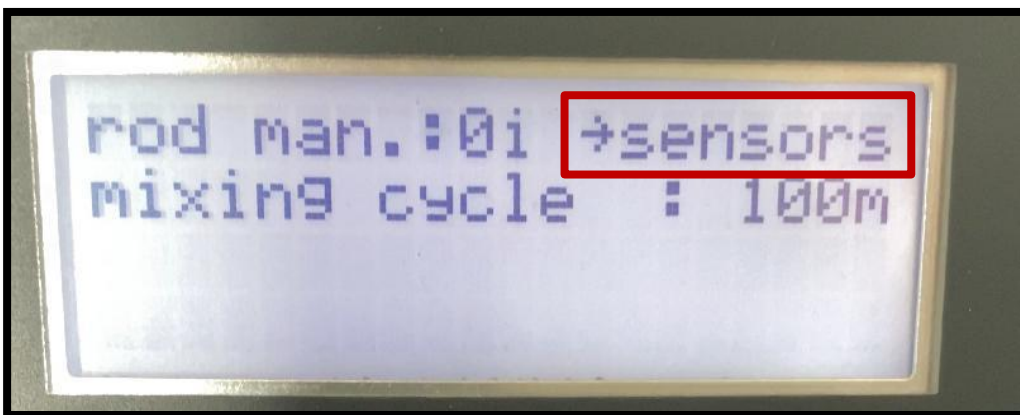


- Press 'Enter' to go into the **Sensor menu**
- In the **Sensor Menu** press  **Down** and go to the 'Job Code' line

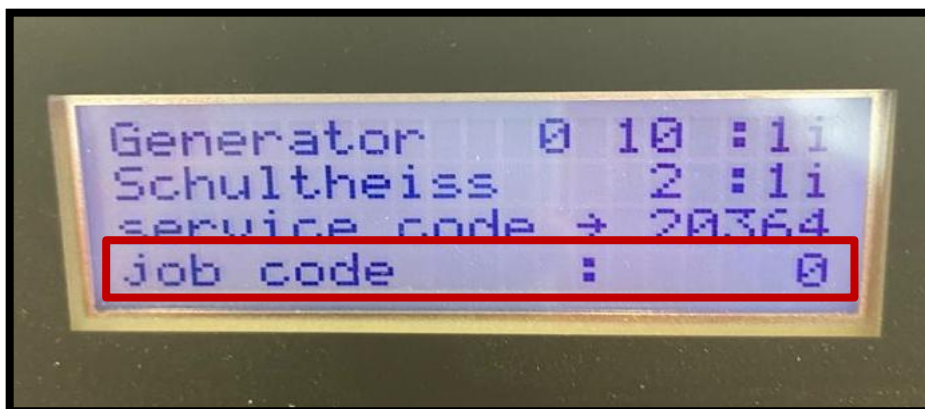


- Press  enter 'Job Code' line

- Press  **Up** to insert the **code : 100**

- Once the code is entered, press  **Enter** to save the code

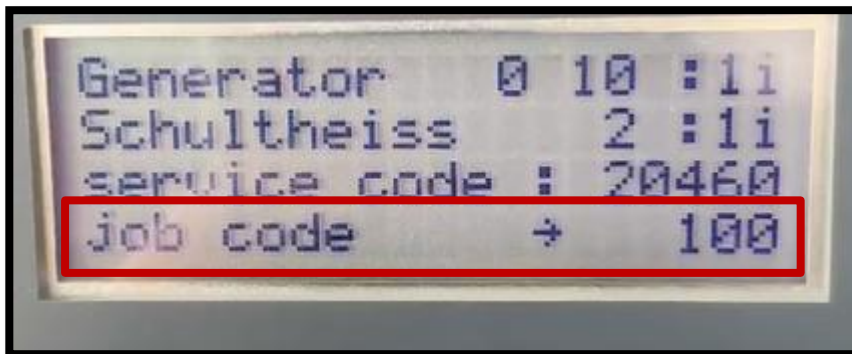

- After the code is entered, the **CLICK** sound of the Valves will be heard multiple times.
- Goto Main menu and the sensor values will be set to 0.00b

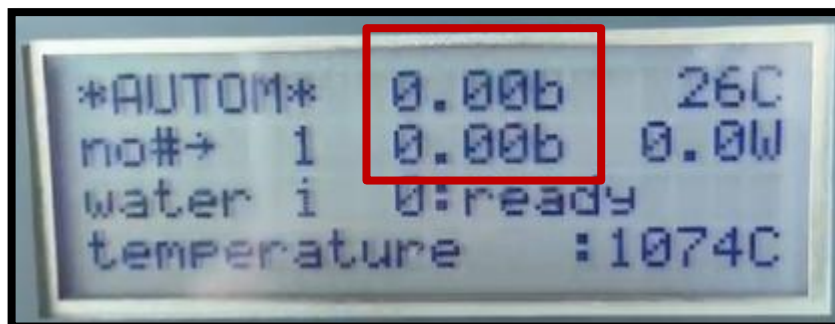

In case the problem still exists, please feel free to contact us again.

E-Mail: service@schultheiss-gmbh.de

Schultheiss GmbH

